



Platinum Nanoparticle in Tantalum Electrode for the Electrochemical Analysis of Heavy Metal Ions formed by the Ion Beam Sputtering Deposition

Ahmad Khalaf Alkhalaf

University of Jordan, Department of Chemistry, Amman - 11942, Jordan

Article History- Received: May 2020; Published: June 2020

Abstract

Today, contamination from heavy metals in the atmosphere is a global concern. Efficient detection techniques are therefore necessary if heavy metal exposure levels in different media are to be determined. The voltammetry method for in situ detection of heavy metal ions is a very sensitive electrochemical method. This thesis explores emerging developments in electrode alteration, materials production and experimental optimization. An electrochemical sensing platinum nanoparticle in the tantalum electrode is provided by means of an Ion Beam Sputtering Deposition (IBSD). The electrode was made with a Pt solution, sputtered simultaneously with hydrochloric acid corrosion on tantalum substrate. In the study of heavy metal ions, for example, the platinum nanoparticle electrodes as prepared were used Square wavelength voltammetry (OSWV) Hg^{2+} , Cu^{2+} and Ag^{2+} . The porous electrodes were observed in a broader range by the Pt nanostructure electrode for heavy metal ions. Furthermore, the susceptibility to detection has been shown to be saturated as the thickness of the layer electrode exceeded 50 nm. For Hg^{2+} 0,003-1 M, for Cu^{2+} 0,005-3 M and for Ag^{2+} the linear detection scale is 0,009-4 M. There has also been good reusability and repeatability. In addition, a scan electron microscope (SEM) used to study platinum electrode forming process and nanostructure. This electrode will have interesting applications in sensing systems.

Keywords: Heavy metal, Platinum electrode, Ion beam sputtering deposition, Nanoparticle.

1. INTRODUCTION

Due to its high degradability, aggregation in live species, which cause diverse diseases and genetic abnormalities, and deleterious ecological consequences, heavy metal ions pose a major threat to human health [1, 2]. First, Pb^{2+} can lead to a wide variety of health conditions, including diarrhea, convulsions, vomiting, and insufficiency of the kidneys, tumors and negative metabolism. [3]. Excessive Cu^{2+} can also be blamed for other illnesses, including hemochromatosis, catarrh, calf cramps, scalp dermatitis brass chills and Wilson's [4]. Several methods have been employed for detecting heavy metal ions, for instance, the use of atomic electron emission spectrometry (ICP / AES, ICP / MS), flow-injection spectroscopy (FIAAS), and high resolution liquid chromatography (HPLC) [5-7]. However, where the concentration spectrum of these metal ions is wide, it is difficult to examine specifically heightened metal ions using these techniques. Therefore, it is urgently necessary to build metal ion sensors with a broader range of detections and high sensitivity. Graphene is a single-atomic layer of tightly packed carbon atoms in a two-dimensional wave [8, 9]. Due to its high electronic mobility, wide surface area and the prevalence of exposed edge planes for greatly raising the storage of charges, platinum has tremendous potential to be used in the production of chemo sensors [10].

The wide range of catalytic, sensor and plasma resonance applications have drawn tremendous attention for porous substances, such as porous gold with a high volume-to-surface ratio, strong electrical and thermal conductivity and a high catalytic performance [11, 12]. Porous gold has recently been shown to be a highly efficient catalyst for many primary reactions such as low-temperature CO oxidation, electrical oxidation, and reduction of oxygen-based hydrogen peroxide [13]. A variety of methodologies have been studied to prepare pore structures, including wet impregnation, relocation, solvent fusion and particulate leaching, rough anodization and magnetron sputtering [14]. Over the years significant advances have taken place in electrochemical science, including the modification of the various types of solid electrodes now being used to test specific sample forms [15]. Recently, the low cost, flexibility and fast adsorption of inorganic materials have drawn significant interest [16]. The most widely used material in electrochemical measurement of heavy metals, particularly nanomaterial-based metals, metal oxides, carbonated metals and their composites [17]. The specific feature of the Ion beam sputtering (IBSD) process is the capacity to deposit high density films at a low substratum temperature through the dynamics for atomic or molecular transport growth mechanism, which gives it numerous benefits including excellent stoichiometry movement, strong durability and simple set-up for the creation of films [18-20]. The platinum

nanoelectrode was rendered in tantalum surface by IBSD and a novel electrode was then used for electrochemical study for detecting of heavy metal ions (Hg^{2+} , Cu^{2+} and Ag^{2+}) in the different mediums.

2. MATERIALS, APPARATUS AND DETECTION OF METAL IONS

Shandong Laiyang Economic and Technologi are bought with hydrochloric acid (37%), neritic acid (98% AR), ammonium acetate (AR), persulfate potassium (AR), oxide phosphate (V) (98%), permanganate potassium (AR), peroxide hydrogen (30%), ethanol (AR), sodium nitrate (AR), and diethyl ether (AR). The Tianjin Aida Hengsheng Manufacturing was acquired with platinum electrode fittings (diameter 6 mm), platinum foil auxiliary and Ag/AgCl reference electrodes. Zhuhai Kaivo Electronic Components purchased tantalum tiles. Qingdao Heli Gas bought ultra-pure nitrogen (99.999%). Flam's ultra-pure water device was developed. Images from a scan-electron microscope were obtained using a JEOL JSM-6700F electron-scan microscope with an accelerated voltage of 5 kV. An EDS detector attached to the above-mentioned SEM microscope, Oxford INCA Sight-X, has been used to carry out energy dispersion testing (EDS). The concustomized three-electrode cell with the electrochemical workstation CHI-760D (CHI Devices, Shanghai, China) was used to perform all electrochemical measurements. At least 15 minutes prior to data collection, the solution had been degassed with nitrogen and blanketed with nitrogen over the completely experimental phase. At room temperatures, all capacity is reached in an electrical one-compartment cell. The IBSD was made of platinum nanoparticle electrode. The electrodes were cleaned thoroughly and dried in oven prior to use with ultra-pure water.

The Square Wave Voltammetry of Oster young (OSWV) has been used in order to illustrate realistic applications of the platinum nanoparticle electrode, to evaluate Hg^{2+} , Cu^{2+} and Ag^{2+} solutions that are more sensitive than differential pulse voltammetry because of the improved reverse reaction sensibility. A mixture of a square wave series with an escalator waveform is the ideal waveform for OSWV. On each square-wave period, the current is sampled twice, one at the end of the forward pulse and one at the end of the opposite pulse. Hg^{2+} , Cu^{2+} and Ag^{2+} solutions were reduced in stock solutions at various rates. The electrodes were washed in an ammonium acetate buffer to ensure complete separation of all the ions with OSWV in transparent solutions of an ammonium acetate buffer.

3. RESULTS AND DISCUSSION

The composition and the cross-section of the electrodes is characterized by the use of SEM testing to ensure the effectiveness of the platinum nanoparticle on the tantalum composition [21]. Fig.1 shows that the electrode is flat and Pt is compacted very tightly. Nevertheless, after hydrochloric corrosion, the microstructure was obtained and pore is distributed similarly. It is very uniform in its dimensions and has a diameter of around 40-75 nm.

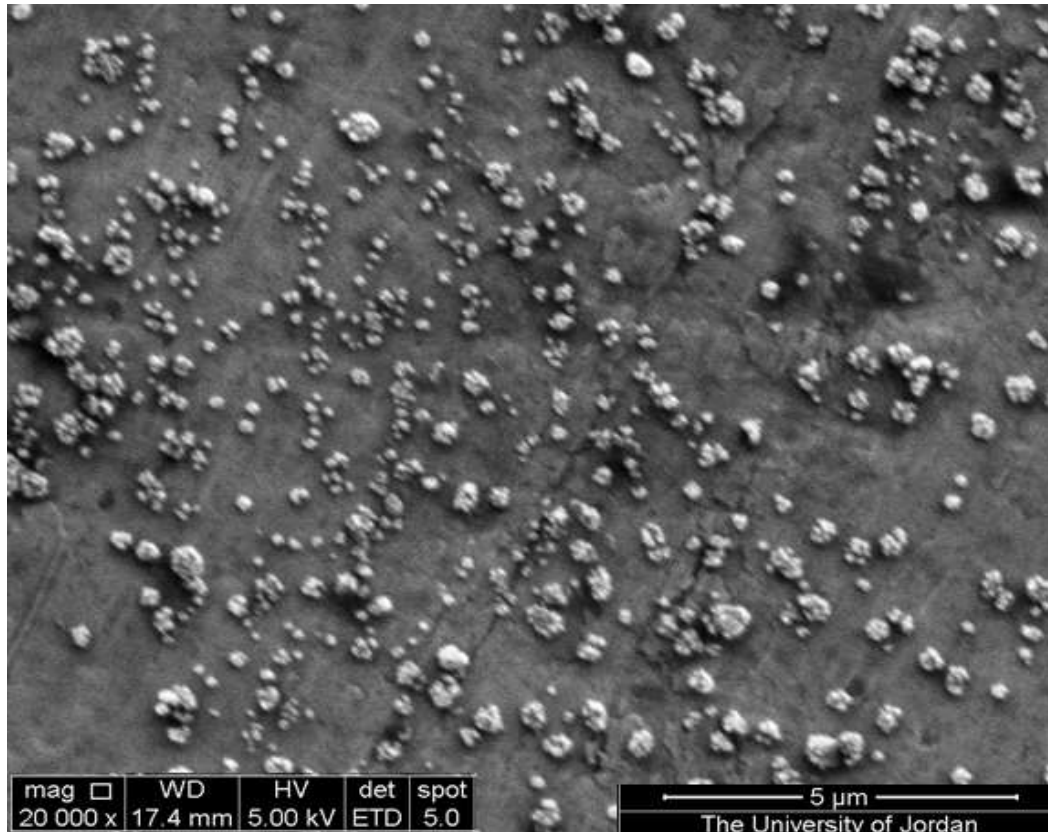


Fig.1 SEM Image of Platinum Nanoelectrode Coated on Tantalum Substrate

In the preparation of the composite target on Ta top, SEM was used to describe the platinum nanoelectrode. In about 150 nm to 1 μm of the SEM picture, the individual platinum surface was nearly translucent. The thickness of this Pt nanoelectrode is relatively uniform, and about 32 nm in diameter, as seen in Fig.1.

An EDX spectrum of deposited particles further confirms the identity of the platinum nanoparticles deposited on a tantalum substrate (Fig. 2). Platinum and tantalum are the main peaks of the EDX spectrum.

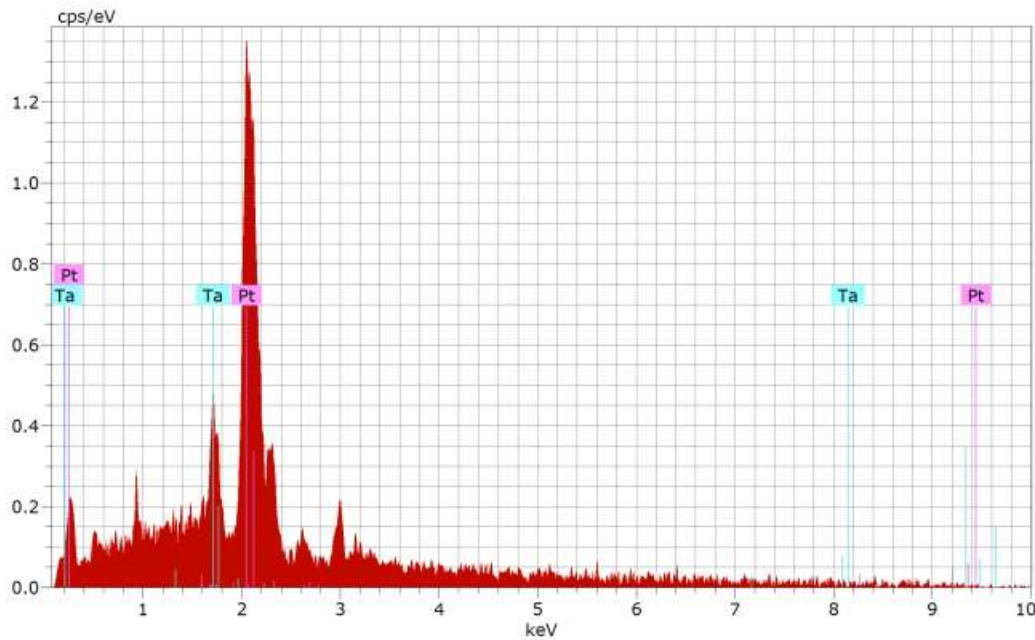


Fig.2 EDX Image of Platinum Nanoelectrode Coated on Tantalum Substrate

One of the most important research techniques for metal ions identification in natural, health and industrial samples is electrochemical research. Possibly, due to special Pt nanostructures and the modern tantalum coating, the electrochemical calculation using platinum nanoelectrode shows enhanced detection range and greatly increased the real area of the electrode allowing more metal ions to react to the electrode.

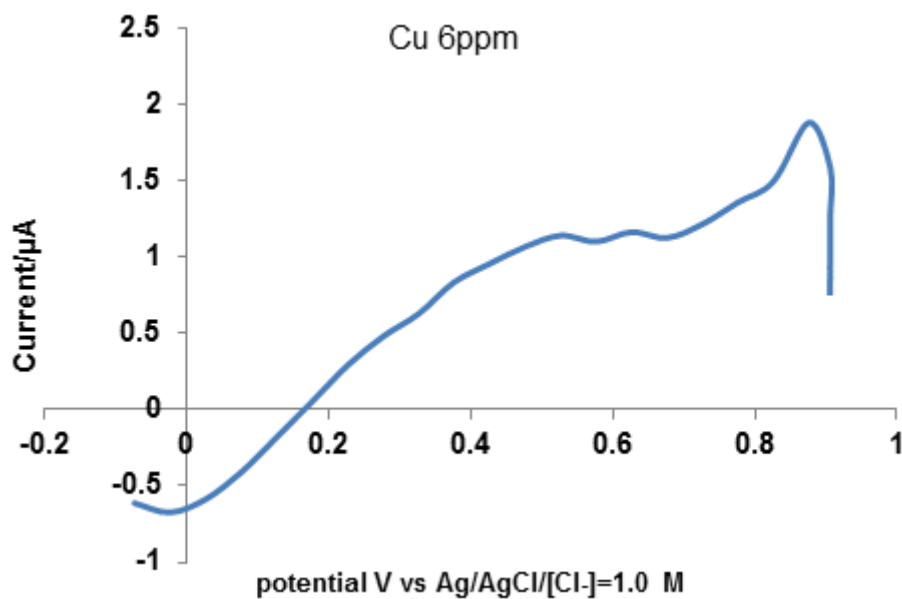


Fig.3 Cyclic Voltammograms of Cu^{2+} solutions with 6 ppm concentration using the Platinum Nanoelectrode at a scan rate of 50 mV s^{-1} .

As shown in Fig. 3, the platinum nanoelectrode detects Cu^{2+} with a buffer solution for ammonium acetate (pH = 5), that is used as a model analytic. Since Oster young square wave voltammetry (OSWV) typically has greater analytical sensitivity, all detections were performed using OSWV in the sample for all heavy metal ions. Cu^{2+} solutions with various rates have been reported from 0.0 V through 0.38 V in a potential window. The prominent peak range from 0.81 –0.92 V to the reference electrode Ag/AgCl has been described to deliver well-defined peaks [22].

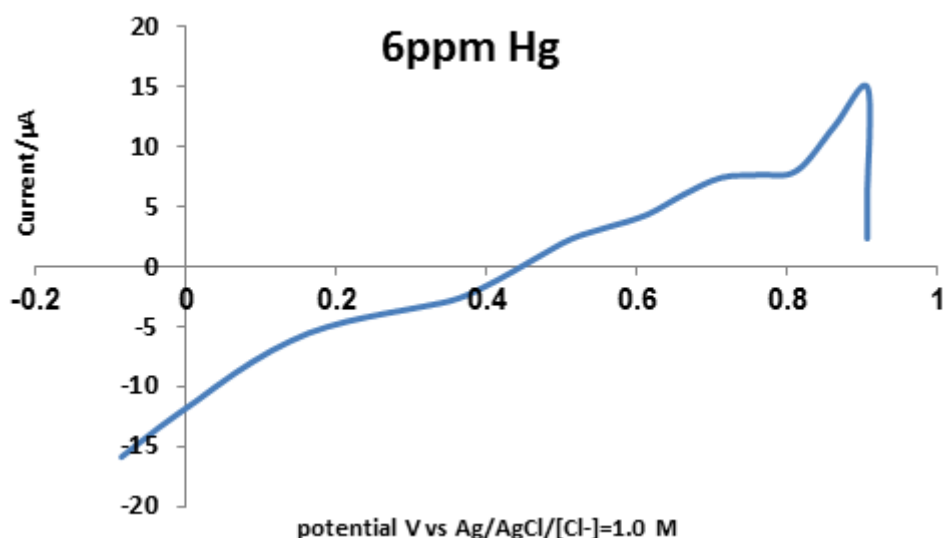


Fig.4 Cyclic Voltammograms of Hg^{2+} Solutions with 6 ppm Concentration using the Platinum Nanoelectrode at a scan rate of 50 mV s^{-1} .

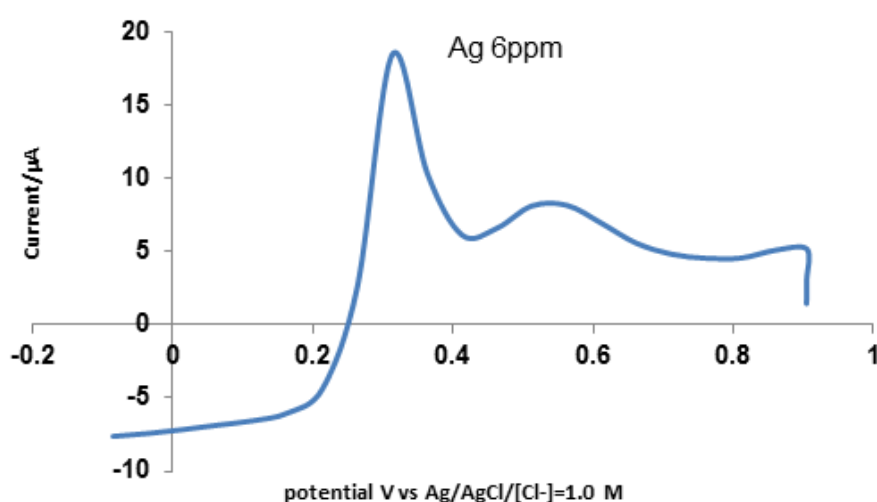


Fig.5 Cyclic voltammograms of Ag^{2+} solutions with 6 ppm concentration using the Platinum nanoelectrode at a scan rate of 50 mV s^{-1} .

Also, in a potential window from Hg^{2+} (0.84 to 0.9 V) Ag^{2+} (0.31-0.39 V) and the use of the platinum nanoelectrode using the OSWV system (Fig. 5 and 6) the Hg^{2+} and Ag^{2+} solutions of different concentration were analyzed.

The reaction of the electrode to Ag^{2+} can be observed as being more active than the detection limit (Cu^{2+} and Hg^{2+}) of 8 nM. Fig. 6 indicates the trajectory of peak current versus concentrations of Hg^{2+} , Cu^{2+} and Ag^{2+} .

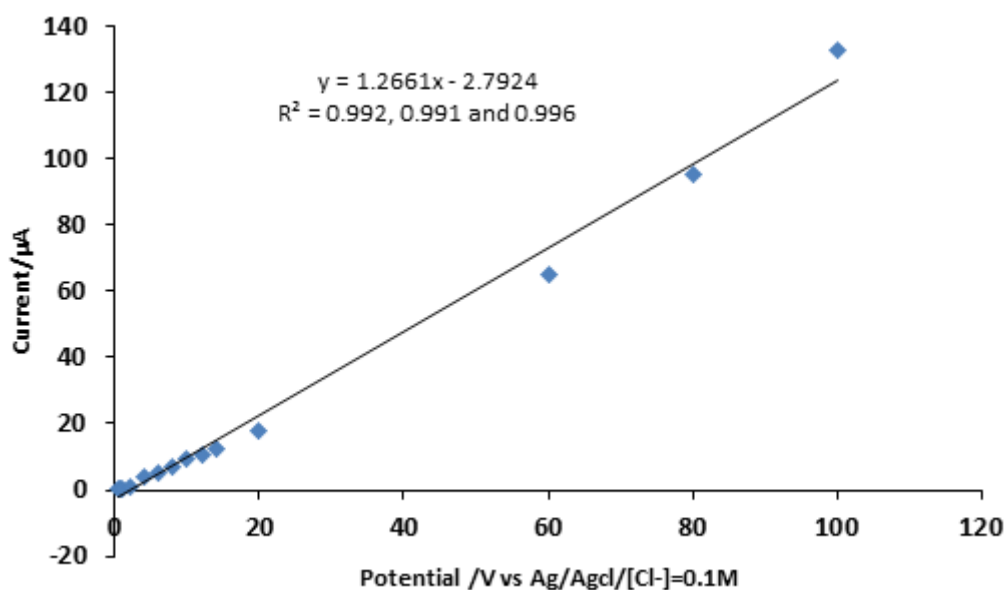


Fig.6 Plot peak current versus concentrations of Hg^{2+} , Cu^{2+} and Ag^{2+} at a scan rate of 50 mV s⁻¹.

The prepared electrode was observed to range from 0.009-4 M, 0.005-3 M and 0.003-1 M respectively to a linear detection of 0.992, 0.991 and 0.996. In contrast, other sensors have previously recorded the detection efficiency of Hg^{2+} , Cu^{2+} and Ag^{2+} . It is clear that the range of detection of our research is superior to other studies, but comparable to some other tests. Platinum nanoparticles electrode stability was tested for 7 days, 14 days and 40 days respectively while keeping the electrodes at room temperature. Platinum nanoelectrode OSWVs have been reported in the ammonium acetate buffer (pH = 5.0) with 2.5 M Hg^{2+} , Cu^{2+} and Ag^{2+} solutions. In the first two weeks, as seen in Fig. 6, just 4.1 percent was deteriorated. After 40 days, the sensitivity of the electrode was still greater than 82.1 % [23].

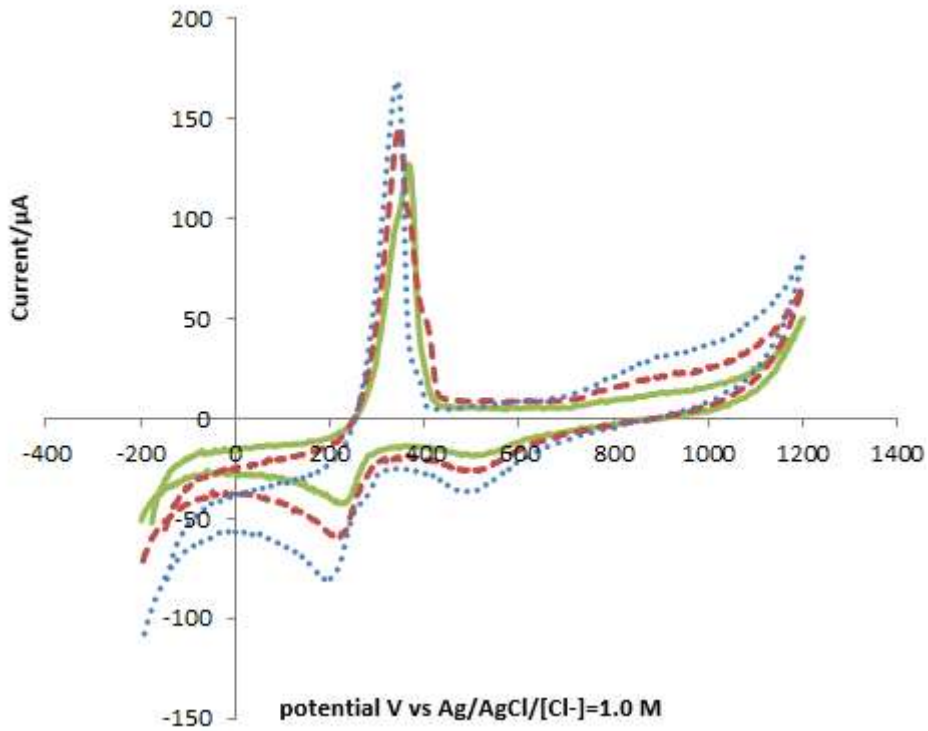


Fig.7 OSWVs of 2.5 M Ag₂+ Ammonium Acetate Solution using the Platinum Nanoelectrode with different days.

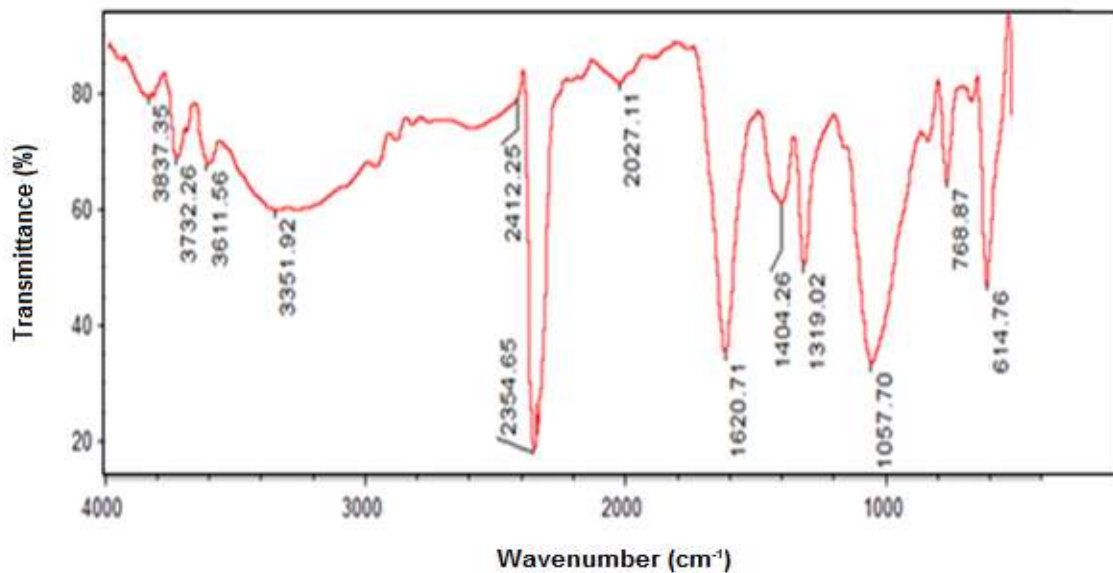


Fig.8 FT-IR spectrum of Hg₂+, Ag⁺ and Cu₂⁺

Ultrasound therapy has also been tested for the stability of platinum nanoelectrode. The sensitivity of Hg₂+, Cu₂⁺ and Ag₂⁺ to detect also exceeded 76.6% by 82.4% and 92.6% after

ultrasonic therapy in the clean ammonium buffer (pH = 5.0), for 10 min [24]. The platinum nanoparticles were found to be solid enough for replicable study in tantalum surface electrodes.

To determine the nature of the sample between surface of electrode and Hg^{2+} , Ag^+ and Cu^{2+} , FT-IR spectra of platinum nanoparticle electrode was recorded in the presence of Hg^{2+} , Ag^+ and Cu^{2+} (Fig. 8). The findings showed that the metal ion Hg^{2+} , Ag^+ and Cu^{2+} was in perfect harmony with the nanoparticulate surface Pt, and the literature published [25].

4. CONCLUSION

In summary, a new method for the manufacture of platinum nanoparticle electrode with a tuning thickness has been successfully produced through ion beam sputters and chemical corrosion. The heavy-metal ion measurement sensitivity was proportional to the pore electrode's thickness and completely saturated after 50 nm. With the added thickness of the porous electrode, the analytical exposure to heavy metal ions is improved. Of Cu^{2+} , 0.005-3 M for the Ag^{2+} analysis and 0.009-4 M for the Hg^{2+} , the linear detection range is 0.003-1 M. Such electrodes were also stable, reusable and anti-interfering.

REFERENCES

1. Xia, Fangquan, Xin Zhang, Changli Zhou, Danzi Sun, Yanmin Dong, and Zhen Liu (2010), "Simultaneous Determination of Copper, Lead, and Cadmium at Hexagonal Mesoporous Silica Immobilized Quercetin Modified Carbon Paste Electrode." *Journal of Automated Methods and Management in Chemistry*, pp.1–6. <https://doi.org/10.1155/2010/824197>.
2. Altweiq, Abdelmnim, and Alkhalaf, Ahmad (2019), "The Determination of Some Heavy Metals in Different Selected Diets". *Eurasian Journal of Analytical Chemistry*, Vol.14 No.4
3. Zhang, Xiao-Lei, Jennifer L Mcglothan, Omid Miry, Kirstie H Stansfield, Meredith K Loth, Patric K Stanton, and Tomás R Guilarte (2017), "From the Cover: 7,8-Dihydroxyflavone Rescues Lead-Induced Impairment of Vesicular Release: A Novel Therapeutic Approach for Lead Intoxicated Children." *Toxicological Sciences*, Vol.161, No.1, pp.186–95. <https://doi.org/10.1093/toxsci/kfx210>.
4. Shi, Yibing, Roumin Wang, Wei Yuan, Qingyun Liu, Mei Shi, Wei Feng, Zhiying Wu, Ke Hu, and Fuyou Li (2018), "Easy-to-Use Colorimetric Cyanine Probe for the Detection of Cu^{2+} in Wilson's Disease." *ACS Applied Materials & Interfaces*, Vol.10, No. 24, pp.20377–86. <https://doi.org/10.1021/acsami.8b07081>.
5. Chaney, Rufus L., Carrie E. Green, and Steven J. Lehotay (2018), "Inter-Laboratory Validation of an Inexpensive Streamlined Method to Measure Inorganic Arsenic in Rice Grain." *Analytical and Bioanalytical Chemistry*, Vol.410, No.22, pp.5703–10. <https://doi.org/10.1007/s00216-018-1075-x>.

6. Terol, Amanda, Eduardo Paredes, Salvador E. Maestre, Soledad Prats, and José L. Todolí (2011), "Alcohol and Metal Determination in Alcoholic Beverages through High-Temperature Liquid-Chromatography Coupled to an Inductively Coupled Plasma Atomic Emission Spectrometer." *Journal of Chromatography*, Vol. 1218, No. 22, pp.3439–46. <https://doi.org/10.1016/j.chroma.2011.03.060>.
7. Martínez, David, Daniel Torregrosa, Guillermo Grindlay, Luis Gras, and Juan Mora (2018), "Coupling Dispersive Liquid-Liquid Microextraction to Inductively Coupled Plasma Atomic Emission Spectrometry: An Oxymoron?" *Talanta*, Vol.176, pp. 374–81. <https://doi.org/10.1016/j.talanta.2017.08.036>.
8. Premathilake, Dilshan, Ronald A. Outlaw, Samuel G. Parler, Sue M. Butler, and John R. Miller (2017), "Electric Double Layer Capacitors for Ac Filtering Made from Vertically Oriented Graphene Nanosheets on Aluminum." *Carbon*, Vol.111, pp.231–37. <https://doi.org/10.1016/j.carbon.2016.09.080>.
9. Wang, Zhong-Xia, and Shou-Nian Ding (2014), "One-Pot Green Synthesis of High Quantum Yield Oxygen-Doped, Nitrogen-Rich, Photoluminescent Polymer Carbon Nanoribbons as an Effective Fluorescent Sensing Platform for Sensitive and Selective Detection of Silver(I) and Mercury(II) Ions." *Analytical Chemistry*, Vol.86, No. 15, pp. 7436–45. <https://doi.org/10.1021/ac501085d>.
10. Hourani, Mohammed Khair, and Alkhalaf, Ahmad (2016), "Synergistic Effects of Bismuth Adatoms on Electrocatalytic Properties of Electrodeposited Nanostructured Platinum Electrodes." *International Journal of Electrochemical Science*, pp.3555–66. <https://doi.org/10.20964/110434>.
11. Zarei, K., and A. Khodadadi (2017), "Very Sensitive Electrochemical Determination of Diuron on Glassy Carbon Electrode Modified with Reduced Graphene Oxide–Gold Nanoparticle–Nafion Composite Film", *Ecotoxicology and Environmental Safety*, Vol.144, pp.171–77. <https://doi.org/10.1016/j.ecoenv.2017.06.030>.
12. Park, Kyungtae, Daheui Choi, and Jinkee Hong (2018), "Nanostructured Polymer Thin Films Fabricated with Brush-Based Layer-by-Layer Self-Assembly for Site-Selective Construction and Drug Release", *Scientific Reports*, Vol.8, No.1 <https://doi.org/10.1038/s41598-018-21493-9>.
13. Saito, Mikiko, Jun Mizuno, Shunichi Koga, and Hiroshi Nishikawa, (2018), "Control for Au-Ag Nanoporous Structure by Electrodeposition and Dealloying" 7th Electronic System-Integration Technology Conference (ESTC), <https://doi.org/10.1109/estc.2018.8546350>.
14. Chiu, Tai-Chia, and Shu-Wei Huang (2018), "Synthesis of Fluorescent Carbon Nanoparticles as Selective and Sensitive Probes for Copper Ions." *Journal of Biosensors & Bioelectronics*, Vol.09. <https://doi.org/10.4172/2155-6210-c1-037>.
15. Wang, Shaopeng, Erica S. Forzani, and Nongjian Tao (2007), "Detection of Heavy Metal Ions in Water by High-Resolution Surface Plasmon Resonance Spectroscopy Combined with Anodic Stripping Voltammetry", *Analytical Chemistry*, Vol.79, No. 12, pp. 4427–32. <https://doi.org/10.1021/ac0621773>.
16. Gao, Chao, Xin-Yao Yu, Shi-Quan Xiong, Jin-Huai Liu, and Xing-Jiu Huang (2013), "Electrochemical Detection of Arsenic(III) Completely Free from Noble Metal: Fe₃O₄ Microspheres-Room Temperature Ionic Liquid Composite Showing Better Performance

- than Gold”, *Analytical Chemistry*, Vol. 85, No. 5, pp.2673–80. <https://doi.org/10.1021/ac303143x>.
17. Cui, Lin, Jie Wu, and Huangxian Ju (2015), “Electrochemical Sensing of Heavy Metal Ions with Inorganic, Organic and Bio-Materials.” *Biosensors and Bioelectronics*, Vol.63, pp.276–86. <https://doi.org/10.1016/j.bios.2014.07.052>.
 18. Xiao, Deli, Siqiao Li, Shubo Liu, Hua He, and Jinrong Lu (2016), “One-Step Hydrothermal Synthesis of Photoluminescent Carbon Nitride Dots Derived from Ionic Liquids.” *New Journal of Chemistry*, Vol.40, No. 1, pp. 320–24. <https://doi.org/10.1039/c5nj01717c>.
 19. Sakiew, Wjatscheslaw, Stefan Schrameyer, Marco Jupé, Philippe Schwerdtner, Nick Erhart, Kai Starke & Detlev Ristau (2019), “Influence of Ion Beam Parameters onto Two-Dimensional Optical Thin Film Thickness Distributions Deposited by Ion Beam Sputtering”, *Thin Solid Films*, Vol. 682, pp. 109–20. <http://doi.org/10.1016/j.tsf.2019.05.027>
 20. Abu-Ali, Hisham, Alexei Nabok, Thomas J. Smith and Maythem Al-Shanawa (2018), “Development of a Novel Electrochemical Inhibition Sensor Array Based on Bacteria Immobilized on Modified Screen-Printed Gold Electrodes for Water Pollution Detection,” <https://doi.org/10.20944/preprints201807.0351.v1>.
 21. Alkhalaf, Ahmad Khalaf, Monzer M.Krishan, Abdelmnim Altwaiq, and Reem Naser Dabaibeh (2020), "Preparation of Nanostructured/ Microplatinum Surfaces by Application of a Square Wave Potential Regime for Methanol Oxidation". *Eurasian Journal of Analytical Chemistry*, Vol.15,No. 1
 22. Cui, Liang, Jingquan Liu, Rui Wang, Zhen Liu, and Wenrong Yang (2012), “A Facile ‘Graft from’ Method to Prepare Molecular-Level Dispersed Graphene-Polymer Composites.” *Journal of Polymer Science Part A: Polymer Chemistry*, Vol.50, No. 21, pp. 4423–32. <https://doi.org/10.1002/pola.26264>.
 23. Pandey, Nidhi, Mukul Gupta, and D. M. Phase (2019), “Preparation and Characterization of Fe₄N Thin Film Deposited by High Power Impulse Magnetron Sputtering.” *Dae Solid State Physics Symposium 2018*. <https://doi.org/10.1063/1.5113132>.
 24. Alshamaileh, Ehab, Mazen Al-Sulaibi, Ahmad Al-Khawaldeh, Mansour H. Almatarneh, Dina El-Sabawi, and Aiman Al-Rawajfeh (2016), “Current Status of Nanotechnology in Jordan.” *World Journal of Science, Technology and Sustainable Development*, Vol.13, No. 2, pp.66–81. <https://doi.org/10.1108/wjstsd-01-2016-0001>.
 25. Zhang, Shanshan, Xingxing Wu, Qingfen Niu, Zongrang Guo, Tianduo Li, and Haixia Liu (2016), “Highly Selective and Sensitive Colorimetric and Fluorescent Chemosensor for Rapid Detection of Ag⁺, Cu²⁺ and Hg²⁺ Based on a Simple Schiff Base.” *Journal of Fluorescence*, Vol.27, No. 2, pp.729–37. <https://doi.org/10.1007/s10895-016-2005-y>.

How to cite this article:

Ahmad Khalaf Alkhalaf, “Platinum Nanoparticle in Tantalum Electrode for the Electrochemical Analysis of Heavy Metal Ions formed by the Ion Beam Sputtering Deposition”, *International Journal of Intelligent Computing and Technology (IJICT)*, Vol.4, Iss.1,pp. 25-35, 2020